



**Kerala State Co-operative Hospital Complex and
Centre for Advanced Medical Services Ltd. No. 4386**

Pariyaram, Kannur, Kerala, 670 503

Email: kchcpariyaram@gmail.com

Phone: 0497-2808111 (15 Lines), Fax: 0497-2808125

No. P2/2382/03/KCHC

07.01.2019

Quotation Notice

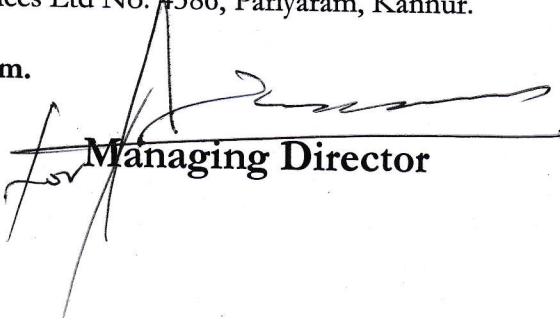
Quotations are invited from the authorized dealers/ companies for the supply of Suction Apparatus in ENT Department in our institution.

Specifications

1. To extract fluid from the body during surgery or emergency treatment
2. Shall have Crompton Greaves/American Universal/GEC Motor of minimum ¼ H.P capacity
3. The machine should be portable on three/four wheels and handle for transportation
4. Suction pump should have line grinding internally
5. The suction pump should be oil immersed fitted on Motor shaft
6. To facilitate maintenance the cover of machine should be easily to open from the top & sides.
7. The suction machine should be capable of producing minimum vaccum of 500 approx mm Hg. Which should be adjustable and monitored by vaccum gauge of suitable range. The suction capacity should be 15 litres per minute and can be regulated.
8. It should have two bottle of 1 or 2 litres (As per requirement) with synthetic rubber lids. The bottle shall be fitted with the arrangement to prevent overflow of fluid.
9. ON/OFF Switch and power indicator should be available
10. Body material: Base, top & panel made of rust proof and corrosion resistant moulded ABS. Jar/Bottle material: Autoclavable polycarbonate.
11. Inbuilt maintenance free battery. Battery backup upto 60 minutes on full charge. Provided with cable for ambulance/car use.
12. 3 core lead of 2 meter along with one 3 pins 15 amp. Plug -01
13. Power cable -3 core lead of 5 meter along with one 3 pins 15 amp. Plug -01
The following spares per machine are also required:-
 - I. Bottles 2 Nos.
 - II. Lids 2 Nos
 - III. Rubber Seals 2 Nos
 - IV. Suction Tubing Set 1 No.
14. Power input to be 220-240 VAC, 50Hz fitted with Indian Plug
15. A fuse or a resettable circuit breaker of a appropriate capacity should be incorporated for protection of motor.
16. Manufacturer/Supplier should have ISO certification for quality standards.

Quotations should be addressed to the Managing Director, Kerala State Co-operative Hospital Complex and Centre for Advanced Medical Services Ltd No. 4386, Pariyaram, Kannur.

Last date of receipt of quotation is 17.01.2019, 4 pm.


Managing Director